

Fig.2

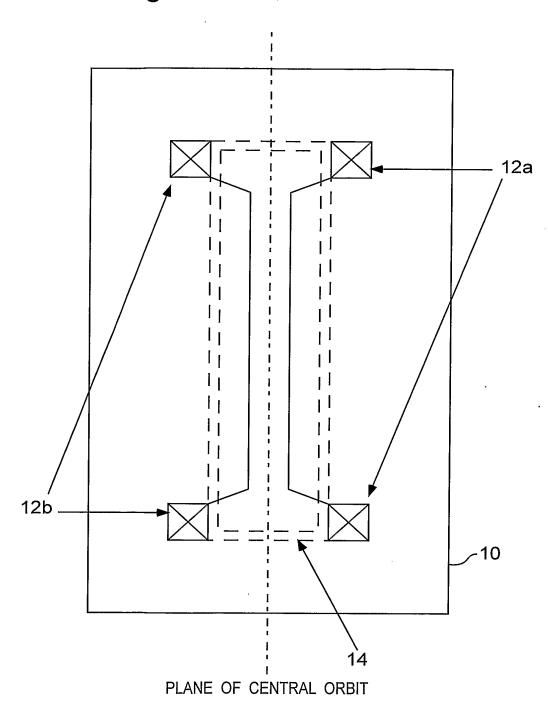


Fig.3


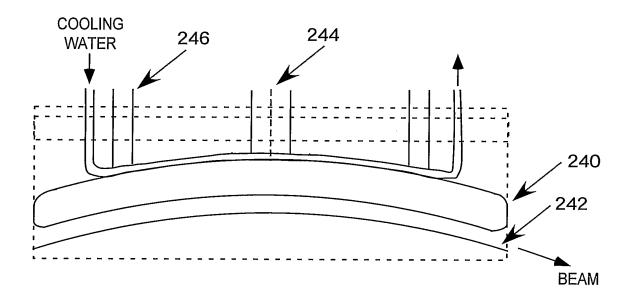


Fig.4



4/8

Fig.5






Fig.6

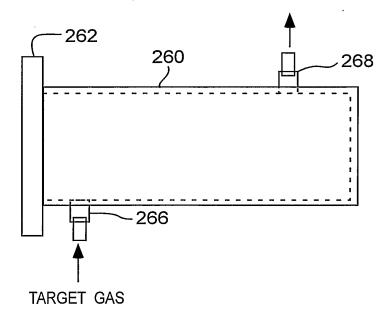

5/8

Fig.7

DOSE EQUIVALENT PER SOLID ANGLE OF DETECTOR E_d =3.5 MeV

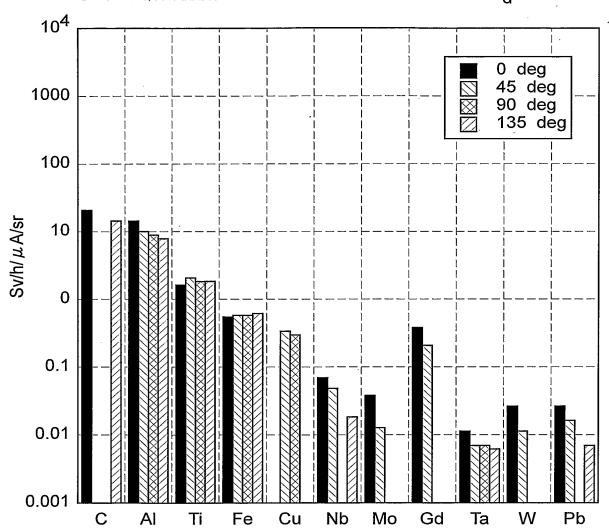

6/8

Fig.8

